

# ERCP sampling devices

---

*“Several studies have shown that the use of multiple ERCP tissue sampling techniques in combination can improve the cancer detection rate.”<sup>1</sup>*

<sup>1</sup>Korc, P. and Sherman, S. “ERCP tissue sampling.” GIE Journal 2016; 84 (4)L 557-571.

An ideal pair, the new **Histoguide™ wire-guided forceps** joins the clinically proven **Infinity® ERCP sampling device**. Pairing the two novel devices for a two-tiered, multi-modality sampling approach may help improve diagnostic capabilities and lead to increased sensitivity during ERCP procedures.<sup>1</sup>


### The Histoguide™ wire-guided forceps...

offers safe and effective placement of forceps into the biliary ductal system along a guidewire to facilitate stricture diagnosis.



### The Infinity® ERCP sampling device...

is proven to be an extremely effective biliary cytology brush delivering a diagnostic sensitivity of up to 85%.<sup>2</sup>

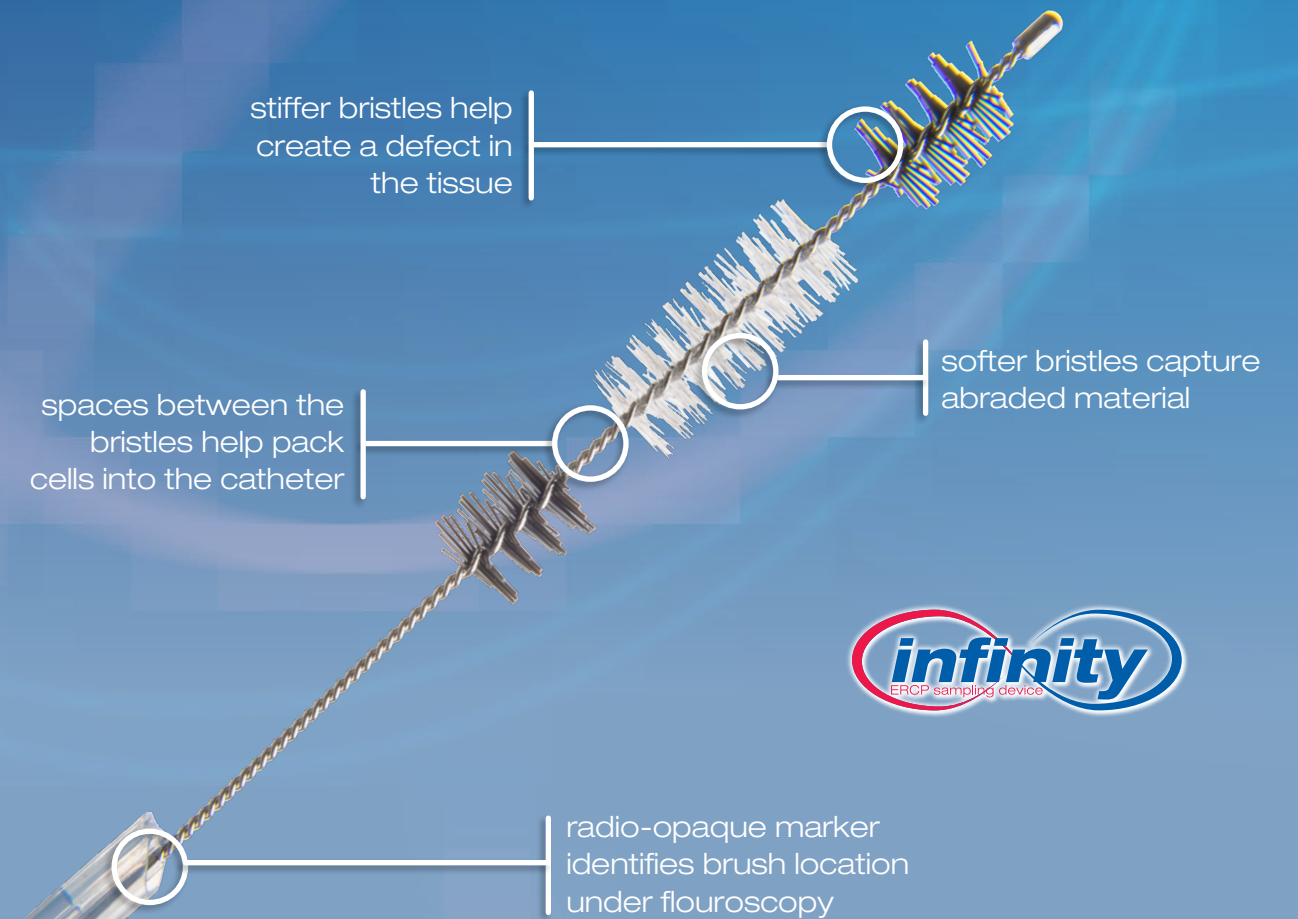

<sup>1</sup>Korc, P. and Sherman, S. "ERCP tissue sampling." GIE Journal 2016; 84 (4)L 557-571.

<sup>2</sup>T. Barrioz, M. Wangermez, P. Levillain, M. Beauchant. The Infinity® brush improves the results of brush cytology for malignant biliary strictures. Societe Nationale Francaise de Gastro-Enterologie (SNFGE). <http://www.snfge.org/jfhod2013/7407.html> [25-4-2013 10:13:01]

### Histoguide™ wire-guided forceps

product number	description	catheter diameter (mm)	wire-guided diameter (mm)	minimum channel (mm)	jaw opening width (mm)	jaw diameter (mm)	length (cm)	units/ box
BX00711660	Histoguide™ wire-guided forceps*	2.1	3.5	4.2	8.0	2.2	230	5

\*Compatible with a .035" guidewire.

### Infinity® ERCP sampling device

product number	description	sheath diameter (mm)	length (cm)	sterile	units/box
BX00711652	Infinity® ERCP sampling device*	3 / 9FR	200	yes	5
BX00711653	Infinity® ERCP sampling device*	2.5 / 7.5FR	200	yes	5

\*Compatible with long and short guidewires.

### ERCP accessories

product number	description	height (cm)	width (cm)	length (cm)	units/ box
BX00711654	Boost® head positioner	9.5	19	23	5

product number	description	dimensions	pouch dimensions	units/ box
BX00711750	Mio® medical device organizer	~86cm x ~76cm	~25cm x ~28cm	20

For more information on our ERCP portfolio, visit [www.usendoscopy.com/ercp](http://www.usendoscopy.com/ercp).

US Endoscopy is a subsidiary of STERIS Corporation.  
 © US Endoscopy or its affiliates. All rights reserved.  
 All marks denoted with ® or ™ are registered with the U.S. Patent and Trademark Office, or trademarks owned by US Endoscopy.  
 US Patent 8,968,213 and other patents pending in the US and other countries.

Follow us:    

5976 Heisley Road  
 Mentor, OH 44060  
 phone (1) 440 / 639-4494  
 fax (1) 440 / 639-4495  
 customer service (1) 800 / 769-8226  
 email [global@usendoscopy.com](mailto:global@usendoscopy.com)  
[www.usendoscopy.com](http://www.usendoscopy.com)